

# VERIFICATION OF CALIBRATION REPORT 1

of Datamaster cdm  
State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program JUN 03 2009

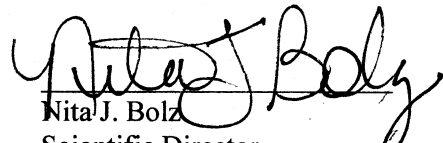
Supervisor/Operator Performing the Verification Procedure:		Datamaster cdm S/N	130180
A	Name	A. W. Anderson	ID# 2467 Date June 1, 2009
	Agency	Seldovia Police Dept.	Phone # (907) 234-7640
	Instrument Location	Seldovia Police Dept.	
B	Alco S/N	X 301530	Target Value .078 High Pressure 600 PSI
	Alco Test Value Average	.078 1 <sup>st</sup> Alco	.076 2 <sup>nd</sup> Alco
	Signature	A.W. Anderson	CRB 6/5/09


(OVER)


(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 12 day of June, 2009.  
 (Notary Seal Stamp)  
Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office



*of Datamaster cdm  
State of Alaska  
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program*

Datamaster cdm S/N

130180 ✓

(CONTINUED FROM FRONT PAGE)

**C**

**TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.**

**NONDRINKING SUBJECT TEST**

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130180

JUNE 01, 2009

OPERATOR'S NAME:

ANDERSON AW

OPERATOR'S NUMBER: 2467

SUBJECT'S LAST NAME:

VERIFICATION OF CALIBRATION

SUBJECT'S FIRST NAME/MI :

N/A

O.L. #: 1234567890

DEPT/AGENCY: SOU1

CASE/REPORT: N/A

TEST TYPE: U

ALCO TARGET VALUE: .078 ✓

ALCO S/N: X301530 ✓

— BREATH ANALYSIS —

.078 ADJUSTED FOR 30.46 in

ALCO TARGET .079 15:08

BLANK TEST .000 15:09

INTERNAL STANDARD VERIFIED 15:09

ALCO TV 30.46 in .076 ✓ 15:10

BLANK TEST .000 15:10

SUBJECT SAMPLE .000 15:11

BLANK TEST .000 15:12

ALCO TV 30.46 in .076 ✓ 15:12

BLANK TEST .000 15:13

**DIAGNOSTIC CHECK**

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130180

JUNE 01, 2009 ✓

TIME 15:03

— DIAGNOSTIC CHECK —

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 41c

BAROMETER: 30.46 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@AB CDEFG  
HIJKLMN OPQRSTU VWXYZ[\]^\_`ab cdefghijklmno  
pqrstuvwxy z{ }~■